

# Performance Analysis of ECG Signal Using Various Window Filtering Techniques

<sup>1</sup>Sabva Rajesh <sup>2</sup>N.B Gohil

<sup>1</sup>Dept. of Electronics & Communication Engineering, Shantilal Shah Engineering college, Bhavnagar  
Gujarat, INDIA

<sup>2</sup>Professor, Dept. of Electronics & Communication Engineering, Shantilal Shah Engineering college, Bhavnagar  
Gujarat, INDIA

<sup>1</sup>[rajeshsabva@gmail.com](mailto:rajeshsabva@gmail.com)

<sup>2</sup>[icc\\_narendra@yahoo.co.in](mailto:icc_narendra@yahoo.co.in)

**Abstract**— ECG signal is of nature of time varying that is most common source used for the diagnosis purpose and observation and analysis of heart diseases present in the patient. ECG is recorded by placing electrodes at specified positions of human body. During recording, ECG is sullied with noises and artifacts which always degrade its quality, and creates accurate and automatic interpretation more difficult. Mostly noticed artifacts or noises are Power line interference, baseline wanders and muscle tremors. So for accurate explanation of characteristics points of ECG, a good quality of ECG is necessary. This paper is presenting a review on various methods for comparing the performance of the digital filter for ECG signal using PSNR, delineation of characteristics points and classification of diseases along with their respective advantages and disadvantages.

**Keywords**— ECG, de-noising, delineation, classification, digital filter.

## I. INTRODUCTION

ECG (electrocardiogram) is a recording of electrical activity of the heart present in human body. In this signal, each heartbeat is represented by an electrical impulse from special cells in right upper chamber of heart. These impulse travels to the other parts of the heart. It then causes the heart to squeeze and pump blood. Finally, it can be detected on the surface of body as ECG patterns [1]. Then, the physician can study the patterns of the recorded signals. There could be several diseases and disorders of various types that affect the ECG pattern. The normal ECG signal wave is given in figure 1.

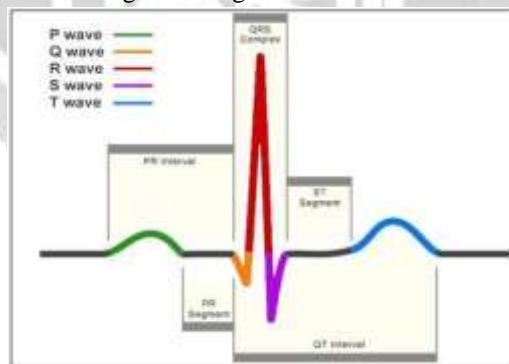


Fig. 1 – Normal ECG Signal Wave.

During recording of ECG from human body, ECG noises (anything other than muscular activity of heart) are superimposed with the recorded ECG [2]. The desired recorded ECG signal can be interrupted due to the presence of AC interference in the power supply, loose electrode connections, malfunctioning of recording machine and sometimes even due to patient movements such as respiration etc. Collectively, these can be labeled as artifacts. Baseline wander, power line interference and muscle tremors are mostly noticed

artifacts/noises. So for accurate delineation of characteristics points of ECG, these artifacts must be removed so that it can be used for proper diagnosis. In the present paper, the survey is based on some of the approaches used for analysis of de-noising ECG signal using FIR-IIR filtering [3].

## II. NOISE IN ECG

In context to ECG signal, noise does not mean sound, although there is analogy between these two terms, but instead to electrical interference. In electrocardiography, rather than using the term noise, the term artifact is more suitable to point out something that is not "heart-made" [4]. The word artifact is alike to artificial in the sense that it is frequently used to indicate something that is synthetic (i.e. not natural). These are electrical disturbances created by electrical noise from elsewhere in the body i.e. any outside sources, placement or poor contact of leads, and machine malfunctions. Artifacts removal is primer requirement to prevent misinterpretation of a heart's rhythm. These are of following types-

### A. Power-Line Interference (Or AC Interference)

Power line interference consists of 50/60 Hz AC (Alternating current) pickups and harmonics present in the power supply. AC more precisely describes the type of electricity that can be obtained from the power line. The electricity frequently changes its direction by 60 Hz power supply in the United States [5]. It is 50 Hz of AC electricity in India and Europe. Major factors that cause such interferences are:

Stray effect of AC fields induced because of loops in electricity cables.

Disconnected electrodes.

Unconventional grounding of ECG machine

Presence of electrical devices in input circuits of ECG machine such as X-ray machines, air conditioner that draws heavy power line current.

Electromagnetic interference generated from the power-line supply.

### B. Baseline Wandering

In baseline wandering, the iso-electric line changes position that is mainly caused by respiration or the patient movements which creates problems in the detection of signal peaks. Some other possible causes are the moving cables during the reading and even by dirty lead electrodes/wires, loose electrodes, and other variety of things. Due to presence of baseline wander the location of T peaks would be detected higher than that of R peak, which might be wrongly taken as R peak instead. The variation of observed amplitude to the peak to peak ECG amplitude will be of 15% [6].

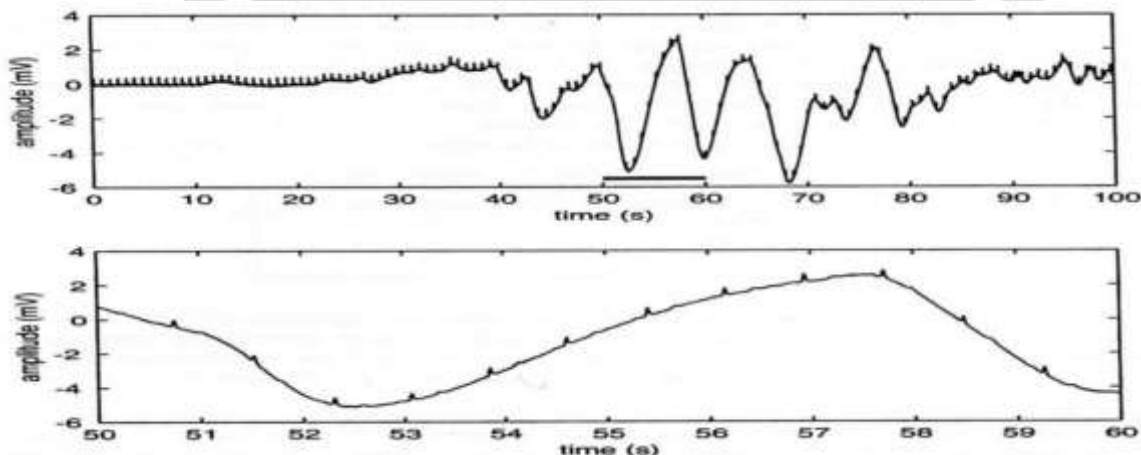


Fig. 2 – Baseline Wander Noise

### C. Muscle Tremor/Noise

Muscle contractions are also called as EMG (electromyography) noise. It is induced by the patient's movement. It generates artifactual milli-volt level potentials as the heart is not the only organ in our body that produces measurable electricity. Even when skeletal muscles undergo tremors there is random activity in the ECG signal. These low amplitude muscle tremor noise can

sometimes mimic the baseline in atrial fibrillation.

#### D. Reversed Leads/Misplaced Electrodes

The placement of electrodes is very important task while recording ECG. The connection between patient and measuring system is interrupted for a short duration due to improper contact of the electrodes which creates electrode contact noise of 1 second duration and amplitude of which is peak recorded output of ECG signal with frequency of 60Hz. Generally, we accidentally get confused with placement of red and white lead cables. When a normal sinus rhythm with all of its waveform upside-down is observed, it is basically a view of the rhythm in a completely different lead [7]. So it's better to reconsider the placements of the electrodes to record clean signal.

#### E. Pacing Spikes

The pacemaker rhythm can easily be recognized on the ECG. These pacing spikes are mainly observed in patients whose implanted pacemaker is firing. These are vertical signal that represents the electrical activity of the pacemaker. The wide QRS complex represents the ventricular depolarization.

#### F. Absolute Heart Block

Absolute heart blockage (also known as 4th degree heart blockage) occurs seldom, only in made-up settings. Spacious and bottle- shaped QRS complexes are observed. The QRS complexes observed here has no relationship with the P wave.

### III. SIMULATION AND RESULT

The implementation of digital filter for ECG artifact removal from Electrocardiogram (ECG) signal are perform in MATLAB.

Phase 1: Firstly we develop a particular GUI for this implementation. After that we develop a code for the loading the input ECG data in the MATLAB database.

Phase 2: Develop a code for the smoothing the input ECG data. After that we got the smooth ECG signal

Phase 3: Develop a code for add noise in ECG signal.

Phase 4: After that we develop code different type of filtering technique



Fig. 3. - Work window of model

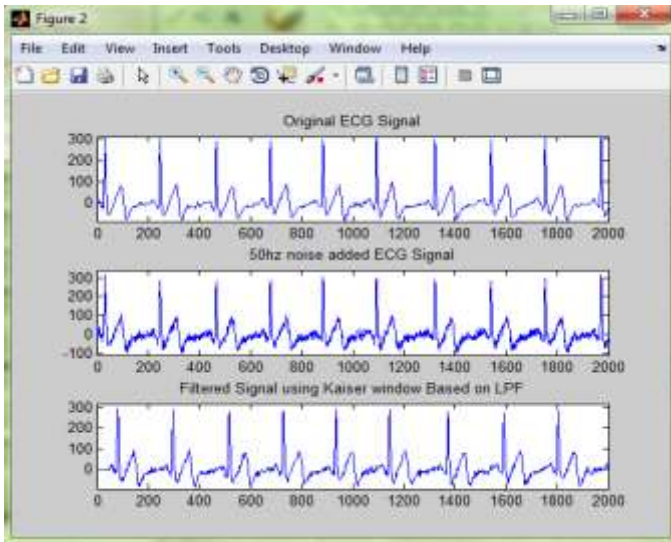


Fig. 4. – Filter signal using Kaiser Window

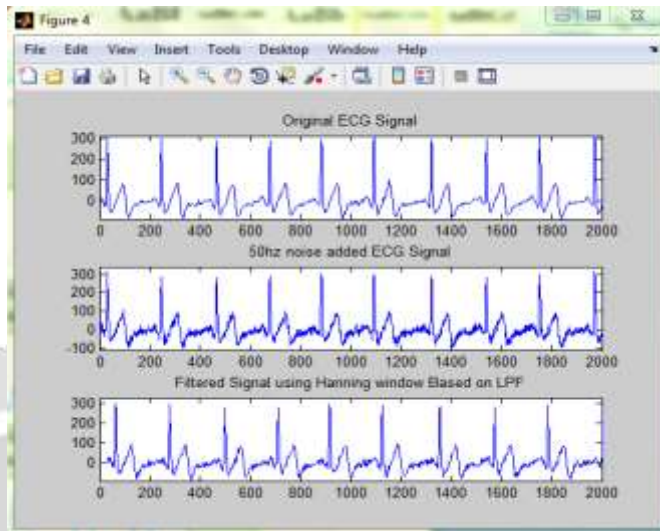


Fig-5-Filter signal using Hanning Window

High Frequency Noise removed from ECG Signal Using Digital Filter. The ECG should be free from noise and of good quality for the correct diagnosis. In real time situations ECG are corrupted by many types of artifacts. The high frequency noise is one of them. The present paper deals with removing of noise from ECG of high frequency contents with help of Low pass digital filter of the cutoff frequency 100Hz. The sampling period used is .001sec. The filter is designed with hanning window of order 100. The results of before filtration and after filtration are depicted in the paper. The experimentation is performed on the database generated in Laboratory. The simulation results show the filter works satisfactorily with some modifications in PQRST waveform.

ECG data sample and original sample are taken as reference signal. The suggested method considers the magnitude response for choosing the cutoff frequency and the FFT spectrum estimate response to find the lowest filter order. The structure and the coefficients of the digital IIR filter are designed using FDA tool in MATLAB. The filter output's average power before and after filtration are calculated using MATLAB and for simulation of this filter, the hardware is designed using raspberry pi. For hardware designing the samples taken are record no. 100 and record no.105 (taken from MIT-BIH database, ML II signal). Here samples are taken from MIT-BIH arrhythmia database (mitdb) ML II are used.

Comparison of Peak Signal to Noise Ratio of Digital Filter.

Filter	Filter Order	PSNR(Peak Signal To Noise Ratio)(DB)
FIR Hamming	100	17.90
FIR Kaiser	100	16.26
FIR Rectangular	100	20.31
FIR Hanning	100	17.65
FIR Blackman	100	18.01



#### IV. CONCLUSIONS

Powerful computer based software tools are commonly used to perform the ECG signal filter. But when we talk about the implementing filter on hardware, the biggest challenge is to achieve specified speed of data processing at minimum hardware cost. The newer paper will present a new design approach to design the digital FIR-IIR digital filter and comparison of their results for filtering artifacts from ECG signal. Then the Filter will be designed, coded using MATLAB and finally implemented on raspberry pi.

#### REFERENCES

- [1] Rakesh Chand, Pawan Tripathi, Abhishek Mathur, K. C. Ray —FPGA Implementation of Fast FIR Low Pass Filter for EMG Removal from ECG Signall. [2] 978-1-4244-8542-0/10/\$26.00 c2010 IEEE.
- [3] Sande Seema Bhogeshwar, M.K.Soni, Dipali Bansal. |Design of Simulink Model to denoise EcG signal using various IIR & FIR filtersl. 978-1-4799-2995- 5/14/\$31.00©20 14 IEEE.
- [4] Kaustubh Manik Gaikwad, Mahesh Shrikant Chavan —Removal of High Frequency Noise from ECG Signal Using Digital IIR Butterworth Filterl. 978-1- 4799-6298-3/14/\$31.00 © 2014 IEEE.
- [5] Rashmi Panda Umesh C. Pati et. al. in —Removal of Artifacts from Electrocardiogram Using Digital Filterl. 978-1-4673-1515-9/12/\$31.00 ©2012 IEEE [6] Savitha R V, S.R.Breasha, X.Felix Joseph —Pre Processing the Abdominal ECG signal using combination of FIR filter and Principal Component
- [7] Analysisl. 978-1-4799-7075-9/15/\$31.00©2015 IEEE.
- [8] Tripti Singh , Prabhakar Agarwal , Dr. V.K. Pandey —ECG Baseline noise removal techniques using window based FIR filtersl. 978-1-4799-5097- 3/14/\$31.00 ©2014 IEEE
- [9] Nalini Singh , Shahanaz Ayub , J.P. Saini —DESIGN OF DIGITAL IIR FILTER FOR NOISE REDUCTION IN ECG SIGNALI. 978 -0-7695-5069-5/13
- \$26.00 © 2013 IEEE DOI  
10.1109/CICN.2013.45

